


To switch panel for  
Loop 1 selection

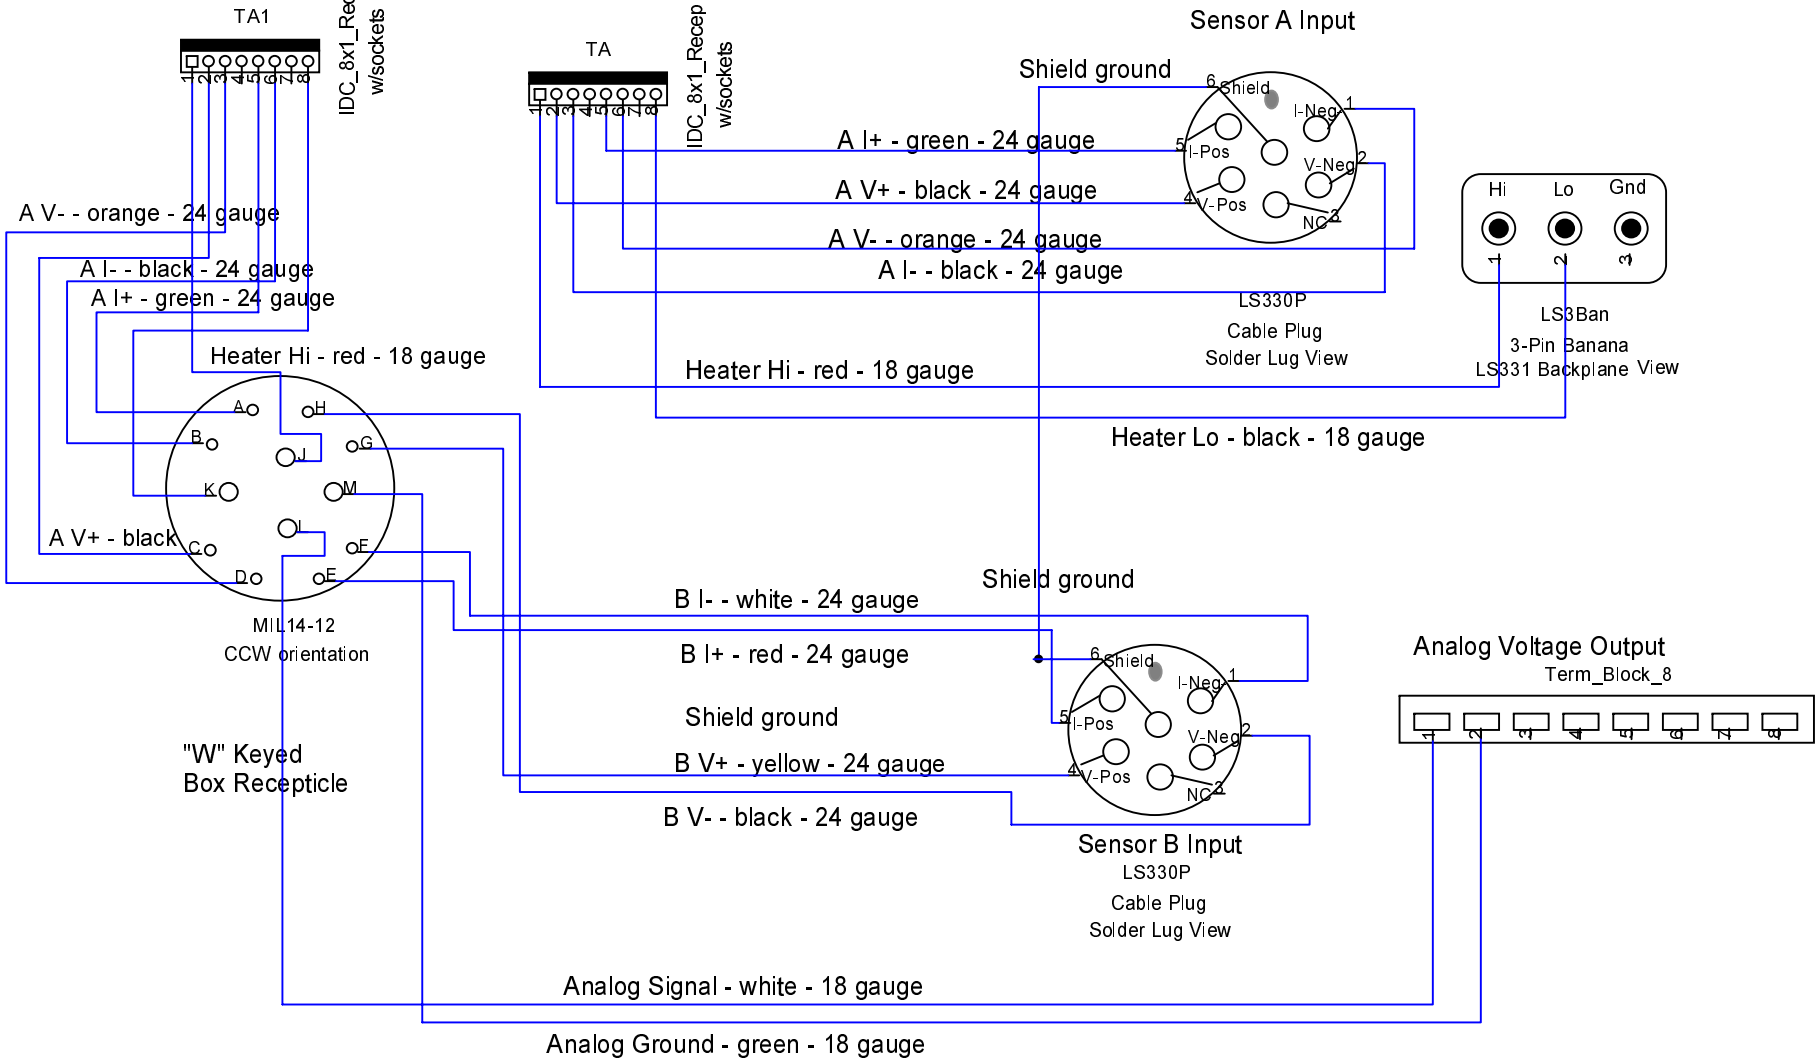

Note: 24 gauge wires are twisted together as pairs within a common shield ground. The heater shield ground is tied to the same sensor shield ground.

LakeShore 331 Temperature Controller to "W" keyed MIL Spec 14-12 box receptacle on electronics box backplane

D. Clemens, Mimir Project, IAR, Boston University, Mod 1.2 J. Shiode, Mod 1.3 D. Clemens

Rev	ID
1.3	5_005_1.3_LS331_to_W_box_receptacle

Date: 2005/03/10

Page: 1 of 1